

Patient: \_\_\_\_\_

Date: \_\_\_\_\_

Notes:

Cephalic Flow

\_\_\_\_\_ ml/min

Basilic Flow

\_\_\_\_\_ ml/min

Basilic

Cephalic

Elbow  
Joint


endoAVF  
Select One

Radial - Radial

Ulnar - Ulnar

### KEY

Cannulation Zone

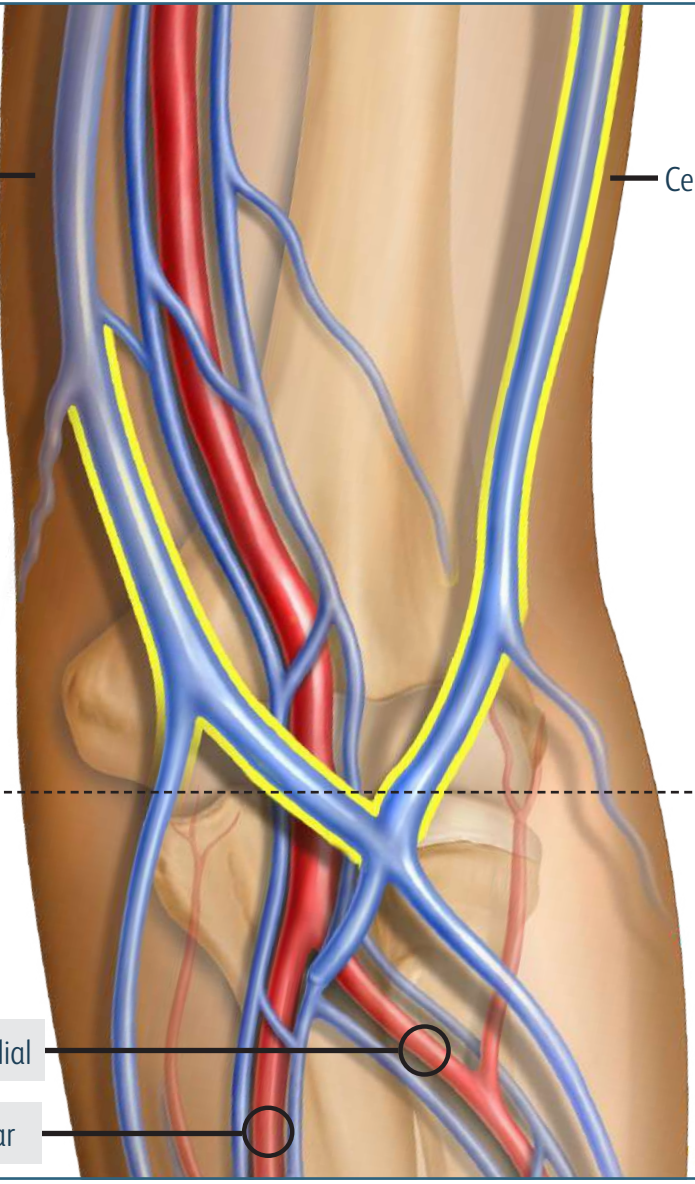

Description:

This diagram represents the flow rates and recommendations for cannulation of the endoAVF.  
If you have any questions, please call the number below:

Name \_\_\_\_\_ Number \_\_\_\_\_

The WavelinQ™ EndoAVF System is intended for the cutting and coagulation of blood vessel tissue in the peripheral vasculature for the creation of an arteriovenous fistula used for hemodialysis. Please consult product labels and instructions for use for indications, contraindications, hazards, warnings and precautions.



[crbard.com/peripheral-vascular](http://crbard.com/peripheral-vascular) | [bd.com](http://bd.com)  
[cannulation@bd.com](mailto:cannulation@bd.com) | [WavelinQsupport@bd.com](mailto:WavelinQsupport@bd.com)

0344

© 2020 BD. BD, the BD Logo, and WavelinQ are trademarks of Becton, Dickinson and Company or its affiliates. Illustrations by Mike Austin. All rights reserved.  
BD Switzerland Sarl, Terre Bonne Park – A4, Route De Crassier, 17, 1262 Eysins, Vaud, Switzerland. BD-35833

