

Right Arm Cannulation Diagram

WavelinQ™

EndoAVF System


Patient: _____

Date: _____

Notes:

Cephalic Flow
_____ ml/min

Basilic Flow
_____ ml/min

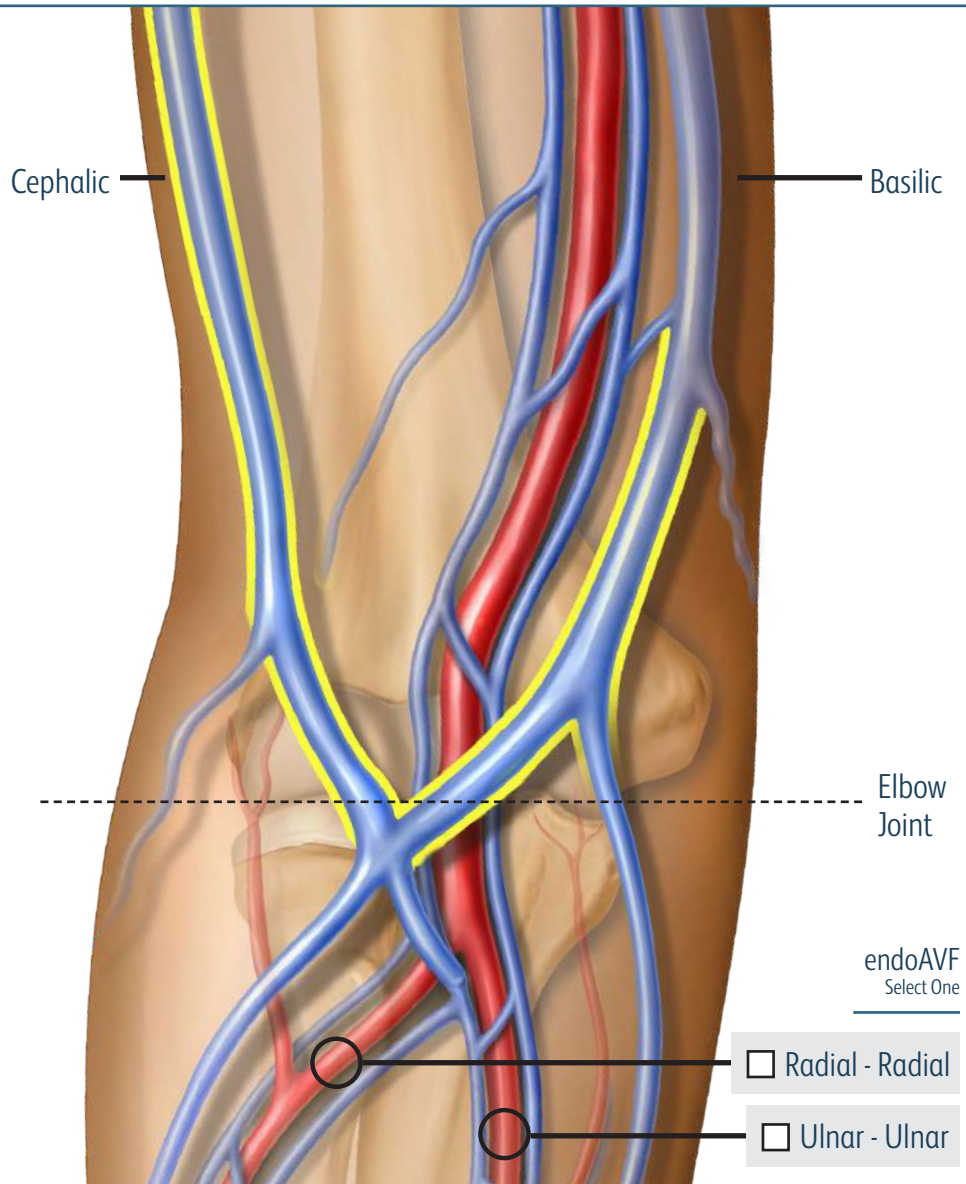

KEY

Cannulation Zone

Description:

This diagram represents the flow rates and recommendations for cannulation of the endoAVF.
If you have any questions, please call the number below:

Name _____ Number _____

The WavelinQ™ EndoAVF System is intended for the cutting and coagulation of blood vessel tissue in the peripheral vasculature for the creation of an arteriovenous fistula used for hemodialysis. Please consult product labels and instructions for use for indications, contraindications, hazards, warnings and precautions.